

3M™ Tegaderm™ I.V. Port Dressings



Tough Treatments Made Easier

Oncology patients are vulnerable—and in the fight against infection, the dressing you use really matters. Tegaderm™ I.V. Port Dressings are specifically designed for implanted venous ports, offering both antimicrobial protection and the comfort your patients deserve.

Tegaderm™
Brand

3M

3M™ Tegaderm™ I.V. Port Dressings

Patient Comfort: Adhesive-free window minimizes adhesive contact with patient skin


Antimicrobial Protection: CHG gel pad provides immediate and continuous antimicrobial protection^{*1,2}

Patient and Clinician Safety: Adhesive-free window reduces risk of dressing sticking to needle during removal

Gentle and Strong: Flexes with patient movement and can be worn up to 7 days

Easy Monitoring: Transparent dressing and CHG gel pad permit clear visibility around the needle insertion site

* Available with 3M™ Tegaderm™ CHG Chlorhexidine Gluconate I.V. Port Dressing
 ** *In vitro* testing shows that the transparent film provides a viral barrier from viruses 27 nm in diameter or larger while the dressing remains intact without leakage.

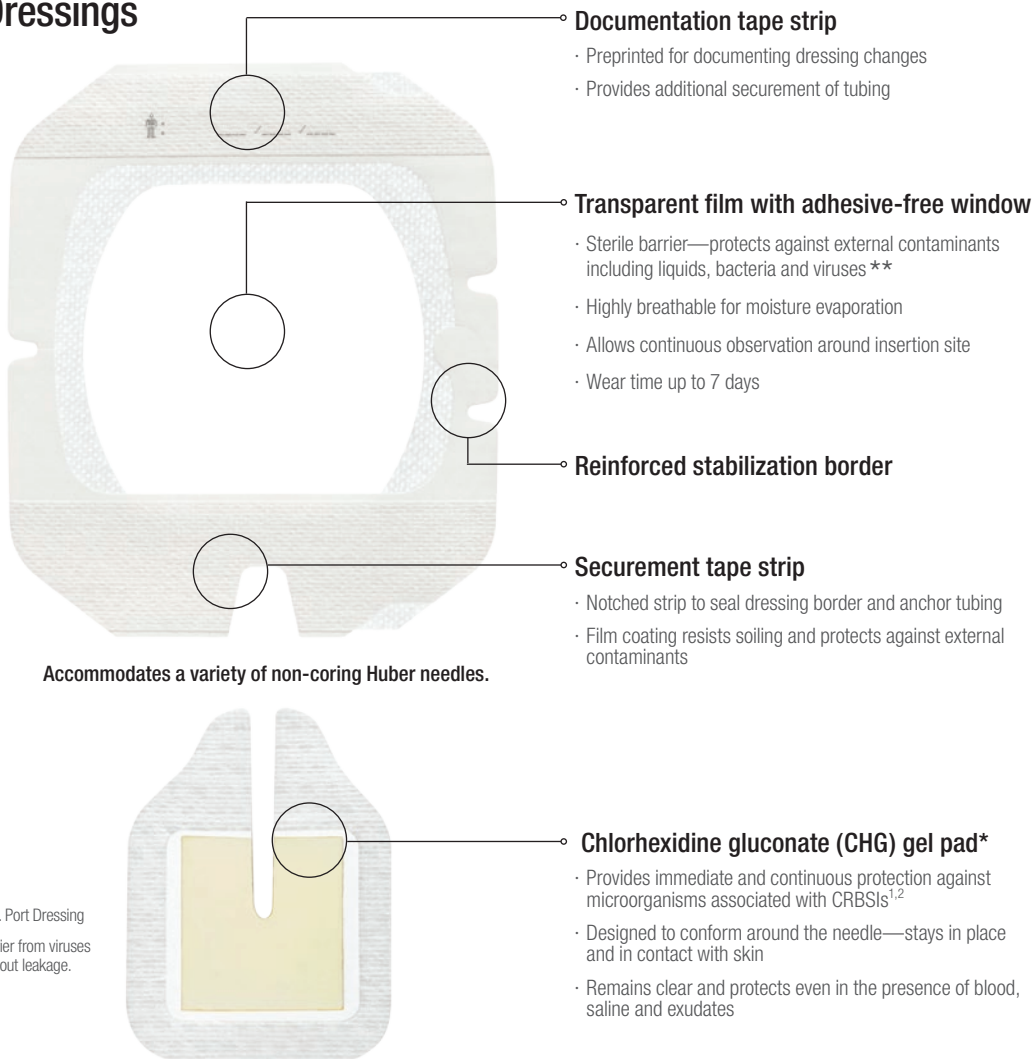

Ordering Information

PRODUCT NAME	PRODUCT CODE	SIZE	EACH/ BOX	BOXES/ CASE	HCPCS CODE
3M™ Tegaderm™ CHG Chlorhexidine Gluconate I.V. Port Dressing	1665	CHG gel pad device 2 7/16 in. x 1 15/16 in. 6,2 cm x 4,9 cm Dressing 4 3/4 in. x 4 3/4 in. 12 cm x 12 cm	25 dressings + devices/box	4 boxes/ case	A6268
3M™ Tegaderm™ I.V. Transparent Film Dressing with Adhesive-Free Window	1668	Dressing 4 3/4 in. x 4 3/4 in. 12 cm x 12 cm	25 dressings/ box	4 boxes/ case	A6268

Disclaimer:
 HCPCS codes have been provided to assist you in the preparation of insurance claims. Please note, however, that the reimbursement information provided by 3M Health Care and its representatives is intended to provide general information relevant to coverage and coding for 3M products. Insurers' reimbursement policies can vary and the use of the codes discussed here does not guarantee that an insurer will cover or pay at any particular level. Health care providers should exercise independent clinical judgment in choosing the codes which most accurately describe the products provided.

